

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE
(Docket No. 15-IS-5286)

Maqbol Patel and David McKone

SERIAL NO.:

FILED:

FOR: **IMAGING SYSTEM ADAPTED TO
PARTIALLY PREPROCESS IMAGE
DATA**

EXPRESS MAIL NO.

EL 282 684 548 US

Date: December 28, 1999

jc678 U.S. PTO
09/473638
12/28/99

Assistant Commissioner for Patents
BOX PATENT APPLICATION
Washington, D.C. 20231

Sir:

Transmitted herewith for filing is the patent application of Inventor(s): Maqbol Patel and David McKone.

For: IMAGING SYSTEM ADAPTED TO PARTIALLY PREPROCESS IMAGE DATA

1. Enclosed are:

- ☒ A Combined Declaration and Power of Attorney signed by each inventor.
- ☒ 6 sheet(s) of drawing(s) (informal).
- ☒ 14 pages of specification including a 1 page abstract, and 4 page(s) of claims (Claims 1-20).
- ☒ An Assignment (including Recordal cover sheet and \$40.00 fee).
- ☐ An associate power of attorney.
- ☒ A Transmittal of Information Disclosure Statement and its enclosures.
- ☐ Priority Document

		Appl'n.	
<u>Docket No.</u>	<u>Country</u>	<u>Serial No.</u>	<u>Filing Date</u>

3. The filing fee has been calculated as shown below, based on the assignee's status as a large entity:

	Claims Presented	Extra Claims	Rate per Extra claim	
Total Claims	- 20		X \$ 18	\$.00
Indep Claims	- 3	0	X \$ 78	\$.00
Basic fee				\$760.00
Multiple dependent claim presented (\$260 if any present)				<u>\$.00</u>
Total Filing fee				<u>\$760.00</u>

4. The following arrangements have been made to pay the filing fee:

- ☒ [X] A check in the amount of \$760.00 to cover the filing fee is enclosed.
- ☐ [] The filing fee is not enclosed. This form does not authorize a charge to a deposit account.
- ☐ [] Please charge our Deposit Account No. 13-0017 in the amount of \$~.
- ☒ [X] The Commissioner is hereby authorized to charge any additional filing fees which may be required under 37 C.F.R. 1.16 for this application and for any amendment thereto, or credit any overpayment to Account No. 13-0017.

5. The Commissioner is hereby authorized to charge payment of the following fees during the pendency of this application or credit any overpayment to Deposit Account No. 13-0017.

- ☐ [] No charges are authorized.
- ☒ [X] Any patent application processing fees under 37 C.F.R. 1.17.

6. Please address all telephone calls to:

at telephone No. (312) 707-8889.

7. Please address all correspondence to:

McAndrews, Held & Malloy, Ltd.
34th Floor
500 West Madison Street
Chicago, Illinois 60661

Date: December 28, 1999


John F. Nethery

Reg. No. 42,928

IMAGING SYSTEM ADAPTED TO PARTIALLY PREPROCESS IMAGE DATA

BACKGROUND OF THE INVENTION

This invention relates to picture archiving and communications systems, and more particularly relates to image viewing and manipulation workstations for use in such systems.

Picture archiving and communication systems (PACS) connect to medical diagnostic imaging devices and employ as components an acquisition gateway between the acquisition device and the PACS, storage archiving units, display workstations, databases, and sophisticated data processors. These components are integrated together by a communication network and data management system. A PACS has, in general, the overall goals of streamlining health-care operations, facilitating distributed remote examination and diagnosis, and improving patient care.

PACS have only recently been introduced to the medical community. A reflection of their recent appearance may be seen in limitations inherent with many of the components used to build a PACS. As an example, the acquisition gateway that acquires examination image data from an imaging modality initially modifies the examination image data by applying a full set of preprocessing functions, for example, FUJI preprocessing functions. The preprocessing functions modify the examination image data for contrast enhancement and frequency enhancements, for example, and the acquisition gateway further converts the resultant image data into a PACS compliant format, for example DICOM format. The preprocessing functions initially applied by the acquisition gateway bar the reapplication of the preprocessing functions at the display workstation. Thus, the display workstations coupled to the PACS are unable to perform sophisticated image modifications possible only through access to the preprocessing functions.

In other words, the display workstations used in PACS are adapted only for viewing fully preprocessed image data and performing limited image modification (e.g., contrast enhancement, edge detection, and cropping only on the image data in PACS compliant format). An initial image preprocessing decision is thereby imposed upon all subsequent viewers of the image, including, for example, doctors who will use the image to diagnose a patient. While a fully preprocessed

image may, in fact, be adequate for a particular examination, such preprocessing eliminates the possibility for custom manipulation of the raw image data as an additional aid in diagnosis.

This invention addresses this problem and provides a solution.

5

BRIEF SUMMARY OF THE INVENTION

5 10 15 A preferred embodiment of the present invention provides, in a picture archiving and communication system (PACS), a method for partial preprocessing of raw image data at an image acquisition workstation connected to the PACS system. The method includes the steps of receiving raw image data from an imaging modality, storing predetermined preprocessing functions applicable to the raw image data, applying at least one and fewer than all of the preprocessing functions to the raw image data to form partially preprocessed raw image data, and transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database. The preprocessing functions are characterized by being modality specific enhancements (e.g., contrast and frequency enhancements) at the beginning of the imaging and display chain.

20 25 A preferred embodiment of the present invention also provides an image acquisition workstation for a picture archiving and communication system (PACS) and for partial preprocessing of raw image data. The image acquisition workstation includes a processing circuit, an imaging modality interface for receiving raw image data, and a software memory coupled to the processing circuit. The software memory stores instructions for receiving the raw image data from an imaging modality, applying at least one and fewer than all of predetermined preprocessing functions to the raw image data to form partially preprocessed raw image data, and transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database.

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 presents a high level block diagram of a PACS system.

Figure 2 illustrates a PACS display workstation for processing raw image data.

Figure 3 illustrates a flow diagram of a method for processing raw image data delivered from an imaging modality.

5 Figure 4 shows a flow diagram of a method for default processing of operator preferences.

Figure 5 depicts a flow diagram of a technique for partially preprocessing raw image data delivered from an imaging modality.

Figure 6 shows a block diagram of an acquisition workstation.

10 DETAILED DESCRIPTION OF THE INVENTION

Turning now to Figure 1, that figure shows a medical data network 100 including an imaging modality 102, an acquisition workstation 104, and a PACS network 106. The PACS network 106 includes a PACS image database 108, a raw image data and preprocessing function database 110 ("preprocessing database 110"), and display workstations 112, 114, 116. A set of operator preferences 118 is stored in the preprocessing database 110.

15 The imaging modality 102 is generally a medical diagnostic imaging device. For example, the imaging modality 102 may be an X-ray imager, ultrasound scanner, magnetic resonance imager, or the like. The imaging modality 102 generates examination image data as a result of an examination. The imaging modality 102 is connected to the acquisition workstation 104 using, for example, a network connection or dedicated interface port.

20 The acquisition workstation 104 acts as a gateway between the imaging modality 102 and the PACS network 106. To that end, the acquisition workstation 104 accepts raw image data from the imaging modality 102. In turn, the acquisition workstation 104 optionally performs preprocessing on the raw image data (as described in more detail below) in preparation for delivering image data to the PACS network 106 for storage in the PACS image database 108 or preprocessing database

110. In operation, the acquisition workstation 104 may convert the raw image data into a DICOM standard format, attach a DICOM header, and the like.

The PACS image database 108 and the preprocessing database 110 are illustrated in Figure 1 for convenience as separate databases. However, they may be a single database, separate databases on an single computer, or separate databases distributed among different computers. In general, the PACS image database 108 stores fully preprocessed images (i.e., those images for which no additional preprocessing functions will be applied). On the other hand, the preprocessing database 110 stores partially preprocessed image data ("raw image data") (i.e., that image data that has not yet been completely preprocessed).

The display workstations 112-116 are coupled to the PACS image database 108 and the preprocessing database 110. Thus, the display workstations 112-116 may retrieve images from the PACS image database 108 for immediate modification and display, or the display workstations 112-116 may retrieve raw image data from the preprocessing database 110. When the display workstations 112-116 retrieve raw image data, however, the raw image data is further modified by preprocessing functions to form resultant image data. The resultant image data may then represent a fully preprocessed image, or may require additional preprocessing before being stored as a fully preprocessed image.

The preprocessing functions are characterized in that they are modality specific enhancements (e.g., contrast or frequency compensation functions specific to a particular X-ray imaging device, for example) applied at the beginning of the imaging and display chain. The preprocessing functions differ from the processing functions applied to fully preprocessed images in that the processing functions are not modality specific and are instead applied at the end of the imaging and display chain.

Turning now to Figure 2, that figure illustrates a PACS display workstation 200 suitable for use in the PACS network 106. The display workstation 200 includes a general purpose processing circuit 202, a PACS network interface 204, a software memory 206, and an image display monitor 208. The PACS network interface 204 is generally implemented as a network card connecting to a TCP/IP based network, but may also be implemented as a parallel port interface, or the like. In particular, the software memory 206 is a raw image and preprocessing function software memory.

Thus, the software memory 206 includes, for execution by the processing circuit 202, instructions for retrieving, from a PACS database, raw image data delivered from an imaging modality. The instructions also allow the operator at the PACS workstation 200 to select a preprocessing function for the raw image data.

5 Once the raw image data and the preprocessing function are determined, the instructions in the software memory 206 allow the processing circuit 202 to apply the preprocessing function to the raw image data to create resultant image data.

As an example, the raw image data may be frequency preprocessed raw image data or contrast preprocessed raw image data. In other words, the acquisition workstation 104 may have already performed a limited preprocessing of the examination image data and stored the results in the preprocessing database 110. In a preferred embodiment, the acquisition workstation 104 applies a subset of predetermined preprocessing functions (e.g., frequency preprocessing functions) to the examination image data, allowing the remaining preprocessing functions (e.g., contrast preprocessing functions) to be applied by the PACS workstations 112-116 that thereby generate a fully preprocessed image. In selecting the preprocessing function, the PACS workstation 200 allow the operator to choose one or more remaining preprocessing functions (e.g., frequency or contrast preprocessing functions) for application to the raw image data to generate resultant image data. The resultant image data may be stored in the preprocessing database 110 for future preprocessing, or, if all preprocessing has been accomplished, the resultant image data may be stored in the PACS image database 108 for future processing and display.

10

15

20

In other words, once the resultant image data has been fully preprocessed, regular image processing algorithms may be applied. The processed resultant image data may then be displayed on the image display monitor 208.

25

One specific example of preprocessing functions are the industry standard FUJI Computed Radiography (CR) modality preprocessing functions. The FUJI preprocessing functions include contrast preprocessing functions and frequency preprocessing functions. The contrast preprocessing functions are characterized by the following parameters: GT (contrast type), GA (rotation amount of GT curve), GC (rotation center for GT), and GS (density shift, the amount of shifting applied to GT). The frequency preprocessing functions are characterized by the following parameters: RN (frequency rank), RE (frequency enhancement), and RT (frequency type). Each preprocessing function may represent a linear or non-linear function, function

30

modification, or function parameter. The preprocessing functions may be applied to raw image data any time prior to the image processing and display.

5 The preprocessing functions may be selected based, for example, on an anatomical region to which the raw image data corresponds. In other words, the preprocessing functions selected may vary depending on whether the raw image data represents, as examples, the head, neck, chest, abdomen, breast, lungs, pelvis, or shoulders. The preprocessing functions may vary for each anatomical region due to the differences in tissue, bone, and blood vessel density and prevalence.

10 The display workstations 112-116 preferably allow their operator to save operator preferences in the PACS system 106 for future retrieval and subsequent application. As an example, the display workstations 112-116 may identify an operator by login name or by querying the operator for an identification code. As the operator works with the preprocessing functions, the operator may develop a preference for application of specific preprocessing functions. The display
15 workstations 112-116 save the operator preferences 118 in, for example, in the preprocessing database 110. When the operator logs in at a later time, the display workstations 112-116 query the database for the operator preferences 118 (e.g., based on login name, or operator ID) and retrieve any preferences found.

20 The display workstations 112-116 may then apply the retrieved operator preferences 118 by default to any raw image data currently retrieved by the display workstations 112-116. The operator preferences 118 may include additional information other than the preferred preprocessing functions, including screen resolution, image layout and position, and color information. Furthermore, the operator preferences 118 may additionally be stored based on anatomical areas of
25 interest. For example, the operator preferences 118 may include the default preprocessing functions to be applied for neck images, and the default preprocessing functions to be applied for chest images.

Turning now to Figure 3, that figure illustrates a flow diagram 300 of a method for processing raw image data, and the software steps executed by the
30 processing circuit 202. At step 302, the processing circuit 202 (e.g., manually under operator control or automatically in accordance with an automated processing script) retrieves raw image data from the preprocessing database 110. Subsequently, the processing circuit 202 selects (manually or automatically) a preprocessing function from the preprocessing database 110 (step 304). During step 306, the processing

circuit 202 applies the preprocessing function to the raw image data. As examples, the preprocessing function may include frequency control preprocessing (step 308) or contrast control preprocessing (step 310).

5 After the preprocessing functions are finished, the processing circuit 202 may then apply additional image processing techniques (e.g., edge detection, edge enhancement, noise reduction, image cropping, contrast enhancement, and the like) to the fully processed resultant image data (step 312). At step 314, the processed resultant image data is displayed.

10 Before an operator at a display workstation 112-116 begins work, the display workstations 112-116 may retrieve and apply default operator preferences. Turning now to Figure 4, that figure shows a flow diagram 400 of the steps that a display workstation 112-116 executes to apply the default operator preferences. At step 401, the display workstation 112-116 identifies the operator using, for example, a login name and password. Next, at step 402, the display workstation 112-116 queries a database for operator preferences 118. If operator preferences 118 do not exist, then processing continues at step 408. If operator preferences 118 do exist, then the display workstation 112-116 retrieves the operator preferences 118 (step 404). Subsequently, at step 406, the display workstation 112-116 applies the operator preferences 118 (e.g., screen resolution, image layout, colors, and the like), and in particular applies the preprocessing function preferences as defaults to the current raw image data that the operator is working with.

25 Continuing at step 408, the display workstation 112-116 allows the operator to continue to preprocess the raw image data and to process fully preprocessed image data. The operator may also adjust the operator preferences, such as screen size, image orientation, preprocessing function preference, and the like. In other words, the display workstation 112-116 allows the operator to establish new operator preferences (step 408). When the operator is finished using the display workstation 112-116, the display workstation 112-116 saves the (possibly new or revised) operator preferences in a database, if the operator so instructs the display workstation 112-116 (step 410).

As noted above, the acquisition workstation 104 may apply a subset of predetermined preprocessing functions (e.g., frequency preprocessing functions) to the raw image data, allowing the remaining preprocessing functions (e.g., contrast preprocessing functions) to be applied by the PACS workstations 112-116 that

thereby generate a fully preprocessed image. Turning now to Figure 5, that figure illustrates a flow diagram 500 of the processing that occurs at an acquisition workstation 104. An initial step (step 502) is taken to store predetermined preprocessing functions at the acquisition workstation 104 (e.g., by storing functions, lookup tables, piecewise linear curve approximations, curve parameter values, and the like).

Next, at step 504, the acquisition workstation 104 receives raw image data from an imaging modality. Subsequently, the acquisition workstation 104 preferably applies at least one, but less than all preprocessing functions to the raw image data (step 506) to form partially preprocessed raw image data. The display workstations 112-116 may thereby complete the image preprocessing on the partially preprocessed raw image data using the flexible preprocessing functions. When the acquisition workstation 104 is finished, it transmits the partially preprocessed raw image data to the PACS network 106 for storage in the preprocessing database 110 (step 508).

Turning now to Figure 6, that figure illustrates one embodiment of an acquisition workstation 600 suitable for use with the PACS network 106. The acquisition workstation 600 includes a processing circuit 602, a PACS network interface 604, and an imaging modality interface 606. The acquisition workstation 600 also includes a software memory 608, and an image display monitor 610. The PACS network interface 604 and imaging modality interface 606 are generally implemented as network cards connecting to a TCP/IP based network, but may also be implemented as parallel port interfaces, proprietary hardwired or wireless interfaces, or the like.

The software memory 608, in particular, is a raw image data preprocessing software memory. Thus, the software memory 608 includes, for execution by the processing circuit 602, instructions for performing the functions described above in the flowchart of Figure 5. In other words, the acquisition workstation 600 receives raw image data over the imaging modality interface 606, partially preprocesses the raw image data to form partially preprocessed raw image data, and transmits the partially preprocessed raw image data through the PACS network interface 604 to the PACS network 106.

The raw image data preprocessing method and PACS workstation of the preferred embodiment thus provide much more extensive and detailed image

modification possibilities to the display workstation operator. The present method and workstation thus remove the initial image preprocessing decisions imposed by prior systems upon all subsequent viewers of the image. Thus, doctors and technicians may perform custom manipulation of the raw image data as an additional aid in diagnosis.

While the invention has been described with reference to a preferred embodiment, it will be understood by those skilled in the art that various changes may be made and equivalents may be substituted without departing from the scope of the invention. In addition, many modifications may be made to adapt a particular situation or material to the teachings of the invention without departing from its scope. Therefore, it is intended that the invention not be limited to the particular embodiment disclosed, but that the invention will include all embodiments falling within the scope of the appended claims.

WHAT IS CLAIMED IS:

1. For a picture archiving and communication system (PACS), a method for partial preprocessing of raw image data at an image acquisition workstation connected to the PACS system, the method comprising:

receiving raw image data from an imaging modality;

5 storing predetermined preprocessing functions applicable to the raw image data;

applying at least one and fewer than all of the preprocessing functions to the raw image data to form partially preprocessed raw image data; and

10 transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database.

2. The method of claim 1, wherein the step of predetermining further comprises predetermining preprocessing functions including at least one frequency preprocessing function and at least one contrast preprocessing function.

15 3. The method of claim 1, wherein the step of applying further comprises applying at least one frequency preprocessing function to the raw image data.

4. The method of claim 3, wherein the step of applying further comprises applying a frequency preprocessing function characterized by at least one of a RN, RE, and RT preprocessing parameter.

20 5. The method of claim 2, wherein the step of applying further comprises applying the at least one contrast preprocessing function to the raw image data.

25 6. The method of claim 5, wherein the step of applying further comprises applying a contrast preprocessing function characterized by at least one of a GT, GA, GC, and GS preprocessing parameter.

7. An image acquisition workstation for a picture archiving and communication system (PACS) and for partial preprocessing of raw image data, the image acquisition workstation comprising:

a processing circuit;

an imaging modality interface for receiving raw image data; and

a software memory coupled to the processing circuit, the software memory storing instructions for:

5 receiving the raw image data from an imaging modality;

applying at least one and fewer than all of predetermined preprocessing functions to the raw image data to form partially preprocessed raw image data; and

transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database.

10 8. The image acquisition workstation of claim 7, wherein the raw image data corresponds to an anatomical region, and wherein the at least one preprocessing function applied to form the partially preprocessed raw image data is selected based on the anatomical region.

15 9. The image acquisition workstation of claim 7, wherein the predetermined preprocessing functions including at least one frequency preprocessing function and at least one contrast preprocessing function.

10. The image acquisition workstation of claim 9, wherein the applying instructions further comprise instructions for applying the at least one frequency preprocessing function to the raw image data.

20 11. The image acquisition workstation of claim 10, wherein the applying instructions further comprise instructions for applying a frequency preprocessing function characterized by at least one of a RN, RE, and RT preprocessing parameter.

25 12. The image acquisition workstation of claim 9, wherein the applying instructions further comprise instructions for applying the at least one contrast preprocessing function to the raw image data.

13. The image acquisition workstation of claim 12, wherein the applying instructions further comprise instructions for applying a contrast

preprocessing function characterized by at least one of a GT, GA, GC, and GS preprocessing parameter.

14. A medical data network comprising:

an imaging modality;

5 an image acquisition workstation;

a PACS network interfaced to the image acquisition workstation, the PACS network comprising a networked PACS image database, display workstation, and preprocessing database, and wherein the image acquisition workstation comprises:

10 a processing circuit;

an imaging modality interface coupled to the imaging modality for receiving raw image data; and

a software memory coupled to the processing circuit, the software memory storing instructions for:

15 receiving the raw image data from an imaging modality;

applying at least one and fewer than all of predetermined preprocessing functions to the raw image data to form partially preprocessed raw image data; and

transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database.

20 15. The medical data network of claim 14, wherein the raw image data corresponds to an anatomical region, and wherein the at least one preprocessing function applied to form the partially preprocessed raw image data is selected based on the anatomical region.

25 16. The medical data network of claim 14, wherein the predetermined preprocessing functions including at least one frequency preprocessing function and at least one contrast preprocessing function.

17. The medical data network of claim 16, wherein the applying instructions further comprise instructions for applying the at least one frequency preprocessing function to the raw image data.

5 18. The medical data network of claim 17 wherein the applying instructions further comprise instructions for applying a frequency preprocessing function characterized by at least one of a RN, RE, and RT preprocessing parameter.

19. The medical data network of claim 16, wherein the applying instructions further comprise instructions for applying the at least one contrast preprocessing function to the raw image data.

10 20. The medical data network of claim 19, wherein the applying instructions further comprise instructions for applying a contrast preprocessing function characterized by at least one of a GT, GA, GC, and GS preprocessing parameter.

IMAGING SYSTEM ADAPTED TO PARTIALLY
PREPROCESS IMAGE DATA

ABSTRACT OF THE DISCLOSURE

In a picture archiving and communication system (PACS), a method is provided for partial preprocessing of raw image data at an image acquisition workstation connected to the PACS system. The method includes the steps of receiving raw image data from an imaging modality, storing predetermined preprocessing functions applicable to the raw image data, applying at least one and fewer than all of the preprocessing functions to the raw image data to form partially preprocessed raw image data, and transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database. An image acquisition workstation for a picture archiving and communication system (PACS) and for partial preprocessing of raw image data is also provided. The image acquisition workstation includes a processing circuit, an imaging modality interface for receiving raw image data, and a software memory coupled to the processing circuit. The software memory stores instructions for receiving the raw image data from an imaging modality, applying at least one and fewer than all of predetermined preprocessing functions to the raw image data to form partially preprocessed raw image data, and transmitting the partially preprocessed raw image data to a PACS network for storage in a preprocessing database.

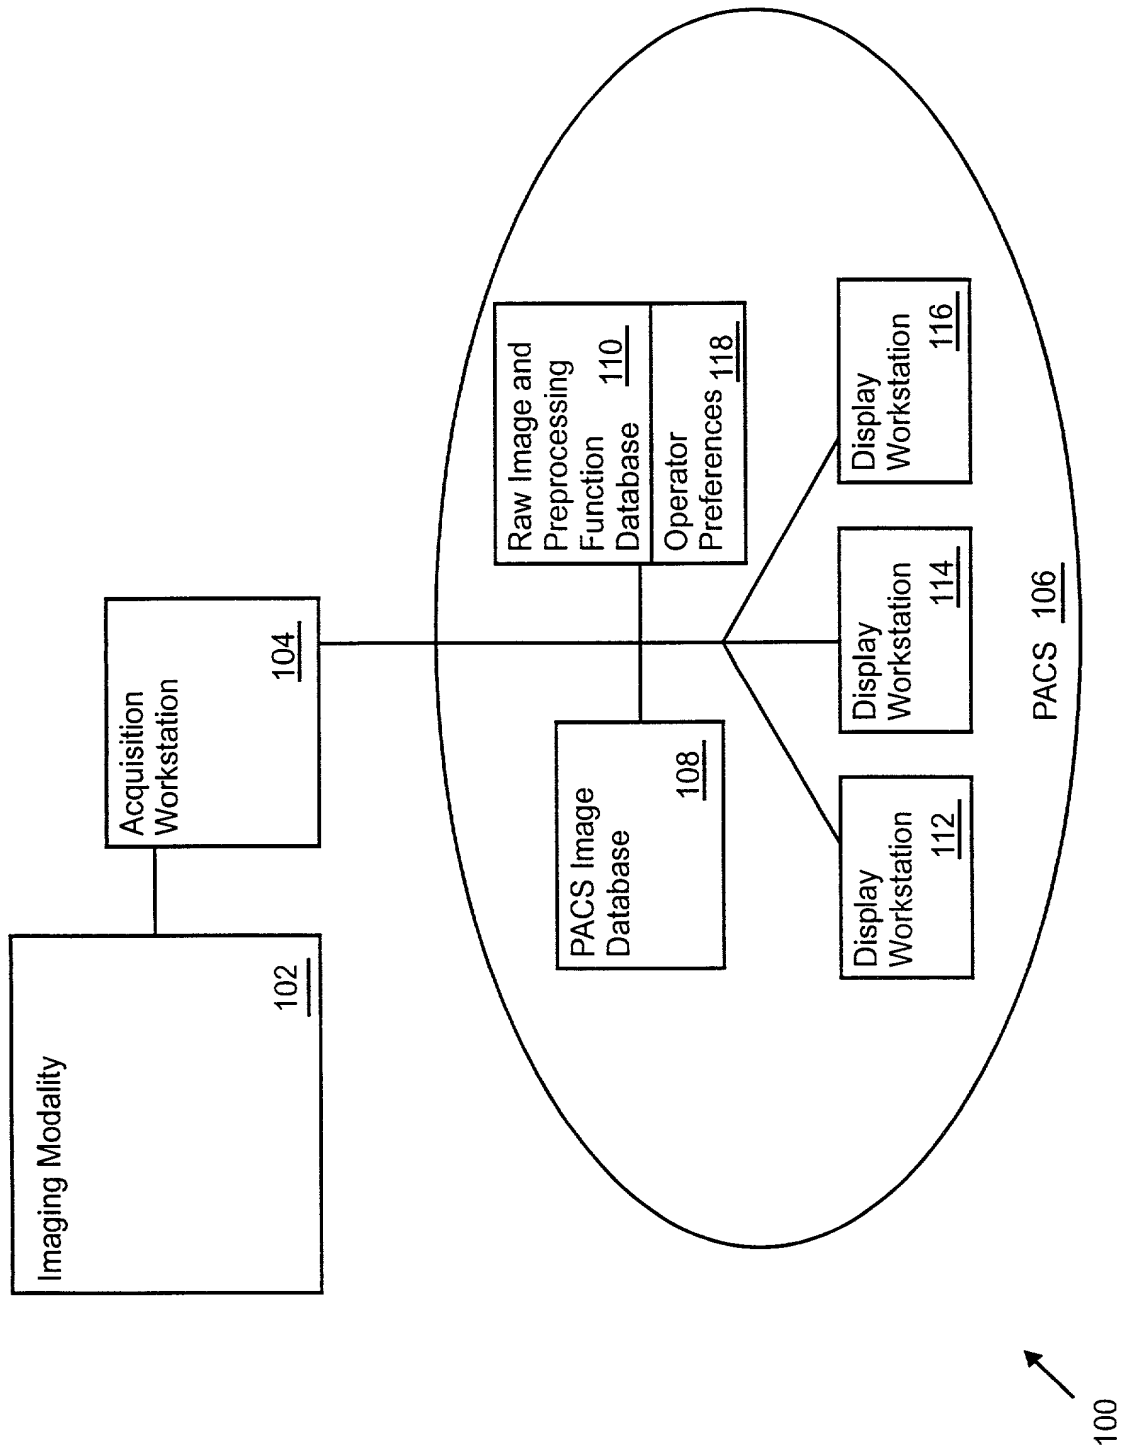


Figure 1

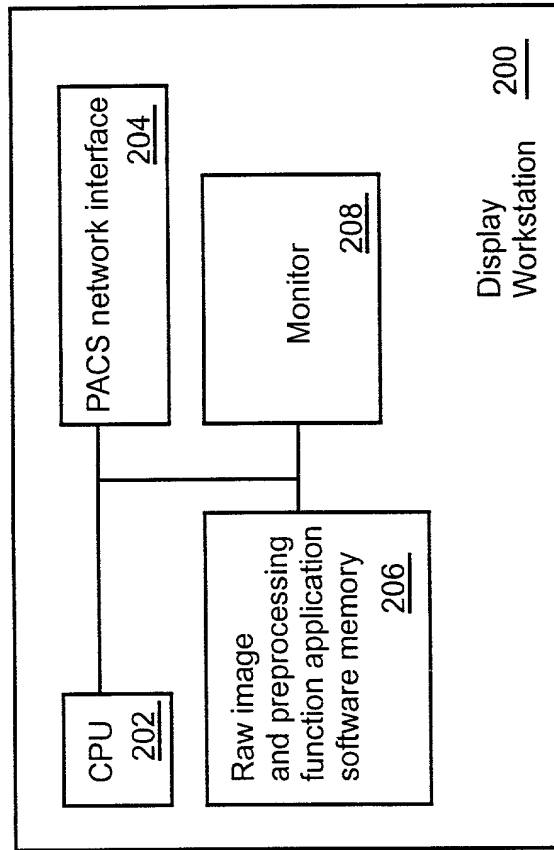


Figure 2


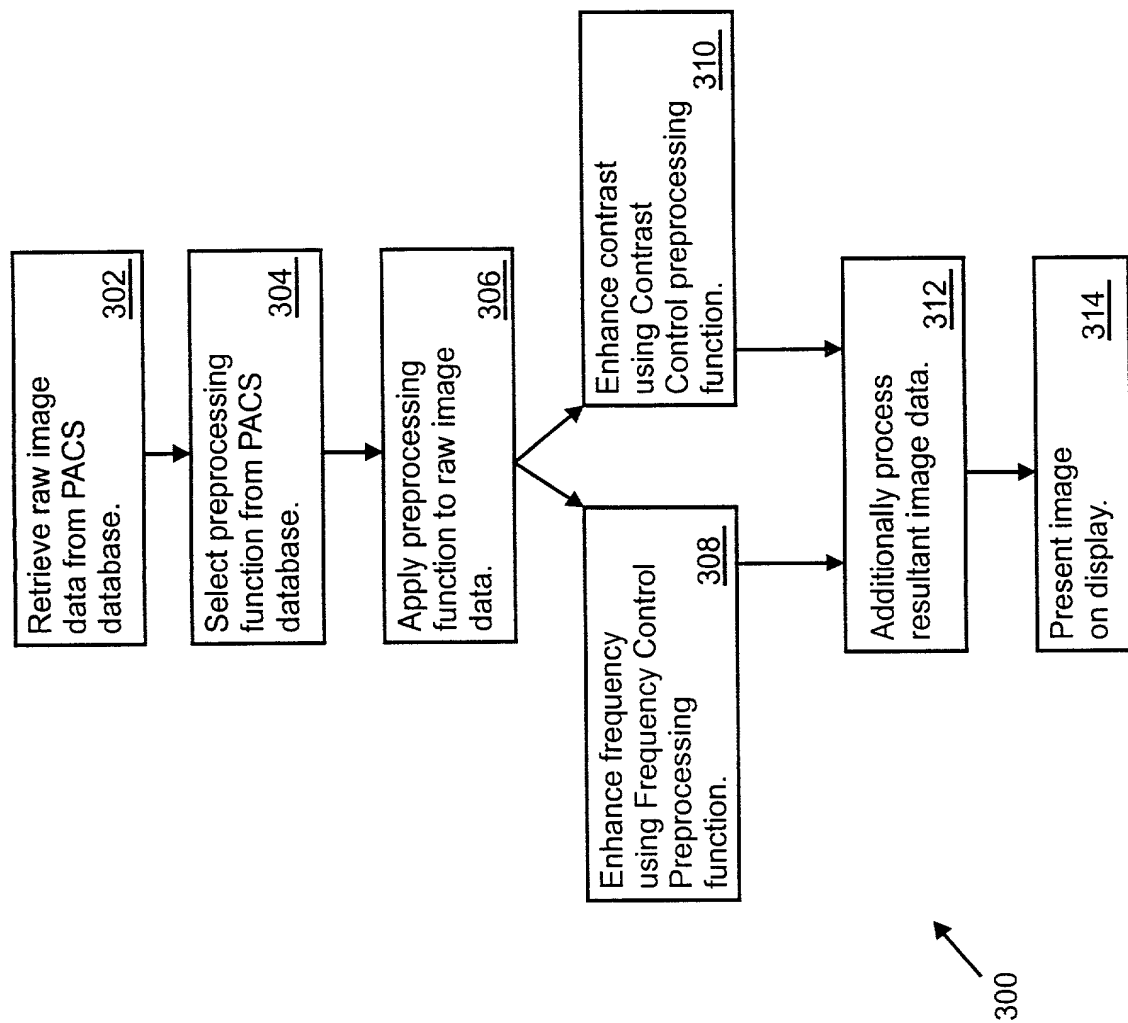


Figure 3



Page 4 of 6

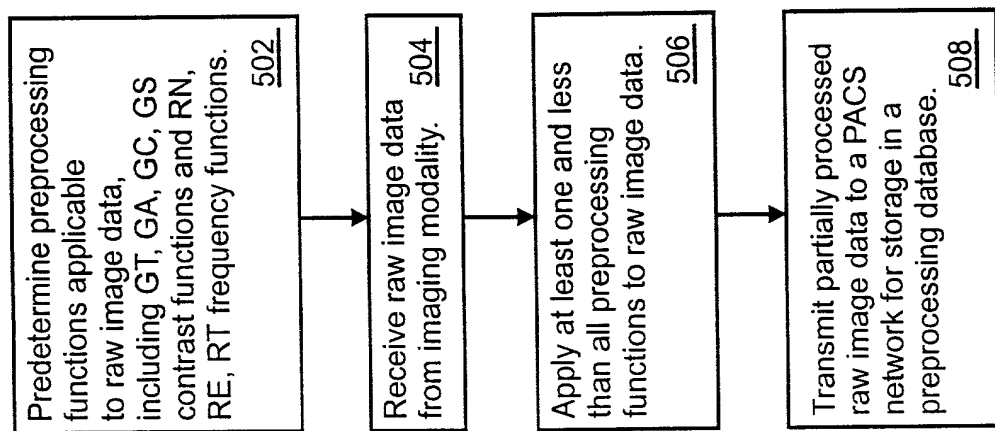


Figure 5

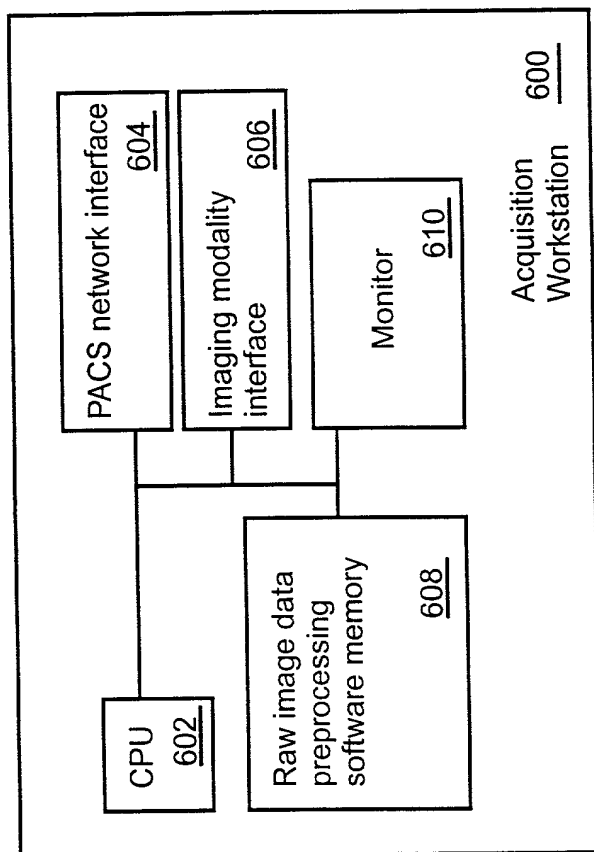


Figure 6

Express Mail No. EL 282 684 548 US

Docket No. 15-IS-5286

**COMBINED DECLARATION AND
POWER OF ATTORNEY FOR PATENT APPLICATION**

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below next to my name.

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled

**IMAGING SYSTEM ADAPTED TO PARTIALLY
PREPROCESS IMAGE DATA**

the specification of which:

☒ X is attached hereto.

* was filed on ~ as United States Application Number or PCT International Application Number ~ and was amended on ~.

I hereby state that I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment referred to above

I acknowledge the duty to disclose to the United States Patent and Trademark Office all information which I know to be material to patentability as defined in Title 37, Code of Federal Regulations, §1.56.

I hereby claim foreign priority benefits under Title 35, United States Code, §119(a)-(d) of any foreign application(s) for patent or inventor's certificate listed below. I have also identified below any foreign application for patent or inventor's certificate having a filing date before that of the application on which priority is claimed.

<u>Number</u>	<u>Country</u>	<u>Day/Month/Year Filed</u>	<u>Is Priority Claimed?</u>
NONE, there are none under Title 35, United States Code, §119(e) of any United States provisional application(s) listed below.			
<u>Application Number</u> <u>Filing Date</u>			
NONE			

659221 "33364460

I hereby claim the benefit under Title 35, United States Code, §120 of any United States application(s) listed below. Insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States application in the manner provided by the first paragraph of Title 35, United States Code, §112, I acknowledge the duty to disclose information which is material to patentability as defined in Title 37, Code of Federal Regulations, §1.56 which became available between the filing date of the prior application and the national or PCT international filing date of this application.

Serial No. Filing Date Patented, Pending, or Abandoned?
 NONE

I hereby appoint the following attorneys and/or agents to prosecute this application and to transact all business in the Patent and Trademark Office connected therewith:

Christian G. Cabou	Reg. No. 35,467
Phyllis Y. Price	Reg. No. 34,234
Ronald E. Myrick	Reg. No. 26,315
Henry J. Policinski	Reg. No. 26,621
Jay L. Chaskin	Reg. No. 24,030
George P. McAndrews	Reg. No. 22,760
John J. Held	Reg. No. 21,061
Timothy J. Malloy	Reg. No. 25,600
William M. Wesley	Reg. No. 26,521
Lawrence M. Jarvis	Reg. No. 27,341
Gregory J. Vogler	Reg. No. 31,313
Jean Dudek Kuelper	Reg. No. 30,171
Herbert D. Hart III	Reg. No. 30,063
Robert W. Fieseler	Reg. No. 31,826
D. David Hill	Reg. No. 35,543
Thomas J. Wimbiscus	Reg. No. 36,059
Steven J. Hampton	Reg. No. 33,707
Priscilla F. Gallagher	Reg. No. 32,223
Stephen F. Sherry	Reg. No. 30,590
Patrick J. Arnold Jr.	Reg. No. 37,769
George Wheeler	Reg. No. 28,766
Janet M. McNicholas	Reg. No. 32,918
Ronald E. Larson	Reg. No. 24,478
Christopher C. Winslade	Reg. No. 36,308
Edward A. Mas II	Reg. No. 37,179
Gregory C. Schodde	Reg. No. 36,668
Edward W. Remus	Reg. No. 25,703
Donald J. Pochopien	Reg. No. 32,167
Sharon A. Hwang	Reg. No. 39,717
David D. Headrick	Reg. No. 40,642

Dean D. Small	Reg. No. 34,730
Alejandro Menchaca	Reg. No. 34,389
Kirk A. Vander Leest	Reg. No. 34,036
Richard T. McCaulley, Jr.	Reg. No. 41,977
Paul L. Rodriguez	Reg. No. 40,788
Anthony E. Dowell	Reg. No. 39,661
Peter J. McAndrews	Reg. No. 38,547
Michael B. Harlin	Reg. No. 43,658
Jonathan R. Sick	Reg. No. 43,920
Krista S. Schwartz	Reg. No. 42,134
Eligio C. Pimentel	Reg. No. 42,076
John F. Nethery	Reg. No. 42,928
Stephen H. Bean	Reg. No. 41,607
Alison L. Pollock	Reg. No. 43,863
James Nuttall	Reg. No. 44,978
James P. Murphy	Reg. No. 40,741
Dean A. Pelletier	Reg. No. 45,007
Joseph M. Barich	Reg. No. 42,291
Tiffany M. Brooks	Reg. No. 44,564
Scott P. McBride	Reg. No. 42,853
Patricia J. McGrath	Reg. No. 44,919
Andrew M. Everest	Reg. No. 44,674
Christopher V. Carani	Reg. No. 44,049

Address all telephone calls to John F. Nethery at telephone number:

(312) 707-8889.

Address all correspondence to:

John F. Nethery
McAndrews, Held & Malloy, Ltd.
34th Floor
500 W. Madison Street
Chicago, Illinois 60661

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

This declaration names 2 inventor(s) below.

Information about sole or first inventor:

(given name, family name): Maqbol Patel

Residence: A-PENI HOUSE, "THE SUMMIT"
SANKEY ROAD
BANGALORE INDIA

Citizenship: INDIAN

Post Office Address: Same

First inventor's signature: Maqbol PatelDate Signed: Dec 24 1999

Information about second joint inventor:

(given name, family name): David McKone

Residence: _____

Citizenship: _____

Post Office Address: Same

Second inventor's signature: _____

Date Signed: _____

Information about sole or first inventor:

(given name, family name): Maqbol Patel

Residence: _____

Citizenship: _____

Post Office Address: Same

First inventor's signature: _____

Date Signed: _____

Information about second joint inventor:

(given name, family name): David McKone

Residence: 4850 Washtenaw Apt C6
Ann Arbor, MI 48108

Citizenship: US

Post Office Address: Same

Second inventor's signature: 

Date Signed: 12/22/99